

**MAA626Hu21**

**Monoclonal Antibody to Caspase 3 (CASP3)**

**Organism Species: *Homo sapiens* (Human)**

***Instruction manual***

FOR RESEARCH USE ONLY

NOT FOR USE IN CLINICAL DIAGNOSTIC PROCEDURES

---

13th Edition (Revised in Aug, 2023)

**[ PROPERTIES ]**

**Source:** Monoclonal antibody preparation

**Host:** Mouse

**Antibody isotype:** IgG2b Kappa

**Purification:** Protein A + Protein G affinity chromatography

**Clone number:** C3

**Traits:** Liquid

**Concentration:** 1mg/ml

**UOM:** 100µl

**Cross Reactivity:** N/A

**Applications:** WB; IHC; ICC; IP.

**[ IMMUNOGEN ]**

**Immunogen:** Recombinant CASP3 (Ser29~Asp175) expressed in *E.coli*

**Accession No.:** RPA626Hu02

**[ APPLICATIONS ]**

Western blotting: 0.01-4µg/mL;

Immunohistochemistry: 5-20µg/mL;

Immunocytochemistry: 5-20µg/mL;

Optimal working dilutions must be determined by end user.

**[ FORMULATION ]**

**Form & Buffer:** Supplied as solution form in PBS, pH7.4, containing 0.02% NaN<sub>3</sub>, 50% glycerol.

**[ STORAGE AND STABILITY ]**

**Storage:** Avoid repeated freeze/thaw cycles.




Store at 4°C for frequent use.

Aliquot and store at -20°C for 24 months.

**Stability Test:** The thermal stability is described by the loss rate. The loss rate was determined

by accelerated thermal degradation test, that is, incubate the protein at 37°C for 48h, and no obvious degradation and precipitation were observed. The loss rate is less than 5% within the expiration date under appropriate storage condition.

**[ IDENTIFICATION ]**

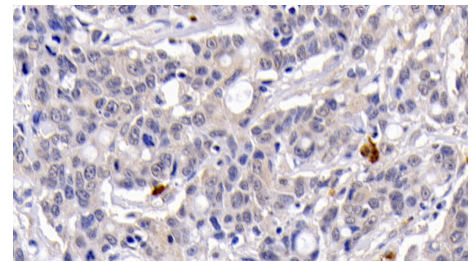


DAB staining on IHC-P;

Western Blot; Sample: Lane1: Human Placenta lysate; Lane2: HeLa cell lysate; Lane3: HepG2 cell lysate; Lane4: Jurkat cell lysate Primary Ab: 0.5µg/ml Mouse Anti-Human CASP3 Antibody Second Ab: 0.2µg/mL HRP-Linked Caprine Anti-Mouse IgG Polyclonal Antibody (Catalog: SAA544Mu19)

Western Blot; Sample: Lane1: Jurkat cell lysate; Lane2: HeLa cell lysate Primary Ab: 4µg/ml Mouse Anti-Human CASP3 Antibody Second Ab: 0.2µg/mL HRP-Linked Caprine Anti-Mouse IgG Polyclonal Antibody (Catalog: SAA544Mu19)

Sample: Human Lymphoma Tissue; Primary Ab: 20µg/ml Mouse Anti-Human CASP3 Antibody Second Ab: 2µg/mL HRP-Linked Caprine Anti-Mouse IgG Polyclonal Antibody (Catalog: SAA544Mu19)

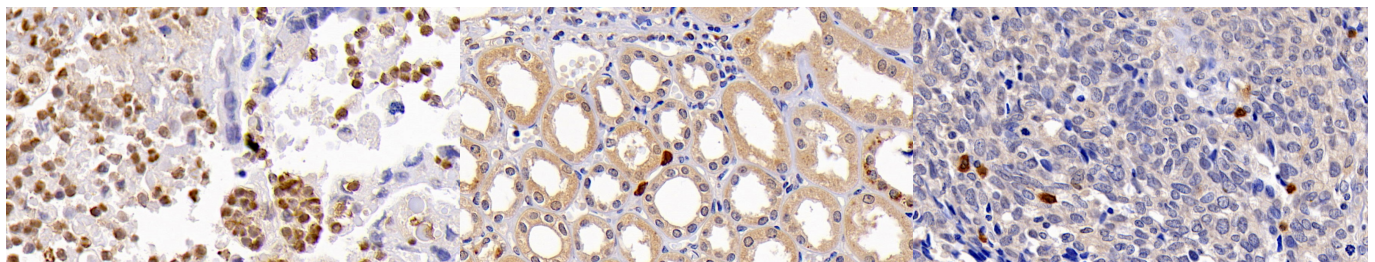

DAB staining on IHC-P;


Sample: Human Lung cancer Tissue; Primary Ab: 20µg/ml Mouse Anti-Human CASP3 Antibody Second Ab: 2µg/mL HRP-Linked Caprine Anti-Mouse IgG Polyclonal Antibody (Catalog: SAA544Mu19)

DAB staining on IHC-P;

Sample: Human Kidney Tissue; Primary Ab: 20µg/ml Mouse Anti-Human CASP3 Antibody Second Ab: 2µg/mL HRP-Linked Caprine Anti-Mouse IgG Polyclonal Antibody (Catalog: SAA544Mu19)

DAB staining on IHC-P;

Sample: Human Ovarian cancer Tissue; Primary Ab: 20µg/ml Mouse Anti-Human CASP3 Antibody Second Ab: 2µg/mL HRP-Linked Caprine Anti-Mouse IgG Polyclonal Antibody (Catalog: SAA544Mu19)

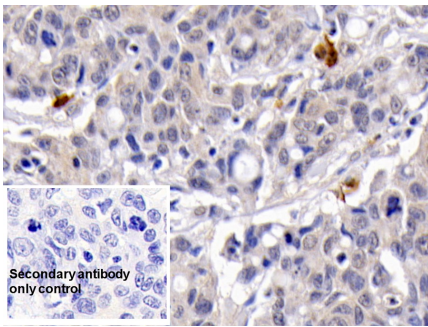

DAB staining on IHC-P;


Sample: Human Lymphoma Tissue

Primary Ab: 20µg/ml Mouse Anti-Human CASP3 Antibody

Control: Used PBS instead of primary antibody

Second Ab: 2µg/ml HRP-Linked Caprine Anti-Mouse IgG Polyclonal Antibody

(Catalog: SAA544Mu19)

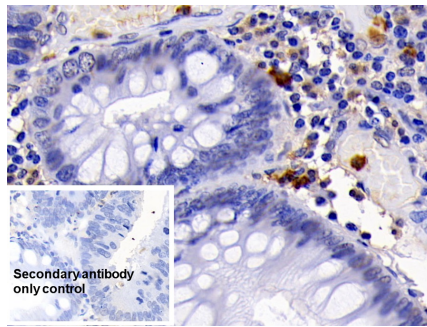

DAB staining on IHC-P;


Sample: Human Colorectal cancer Tissue

Primary Ab: 20µg/ml Mouse Anti-Human CASP3 Antibody

Control: Used PBS instead of primary antibody

Second Ab: 2µg/ml HRP-Linked Caprine Anti-Mouse IgG Polyclonal Antibody

(Catalog: SAA544Mu19)

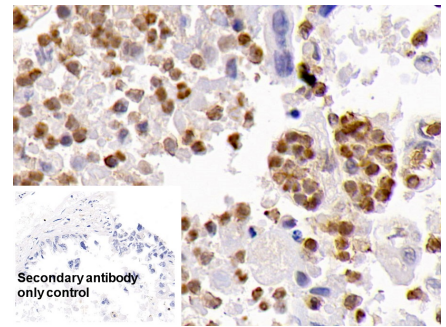

DAB staining on IHC-P;


Sample: Human Lung cancer Tissue

Primary Ab: 20µg/ml Mouse Anti-Human CASP3 Antibody

Control: Used PBS instead of primary antibody

Second Ab: 2µg/ml HRP-Linked Caprine Anti-Mouse IgG Polyclonal Antibody

(Catalog: SAA544Mu19)

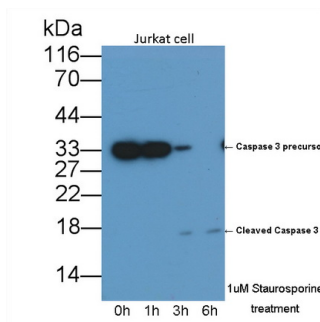

Western blot shows lysates of Jurkat cell line treated with 1 µM staurosporine (STS) for the indicated times.

Primary Ab: 0.02ug/ml Mouse Anti-Human CASP3 Antibody

Second Ab: 0.2µg/mL HRP-Linked Caprine Anti-Mouse IgG Polyclonal Antibody

(Catalog: SAA544Mu19)

**[ IMPORTANT NOTE ]**

The kit is designed for research use only, we will not be responsible for any issue if the kit was used in clinical diagnostic or any other procedures.